


Accessible Round Table Set-Up

Remove two chairs for each mobility device space. Offer multiple choices of where to sit. Increase the amount of accessible seating based on the known or anticipated number of mobility device users expected at your event. Note minimum widths for center and side aisles, and for the distance between accessible and standard rows. Also reduce the number of place settings at a round table by one per mobility device user. Five foot round table: Maximum 8 place settings. Six foot round table: Maximum 10 place settings.



* Measure from the back of one chair to the back of the chair directly behind it. Chairs must be set with the front edge of the chair at the edge of the table. In other words, the chairs should not be pushed under the tables.

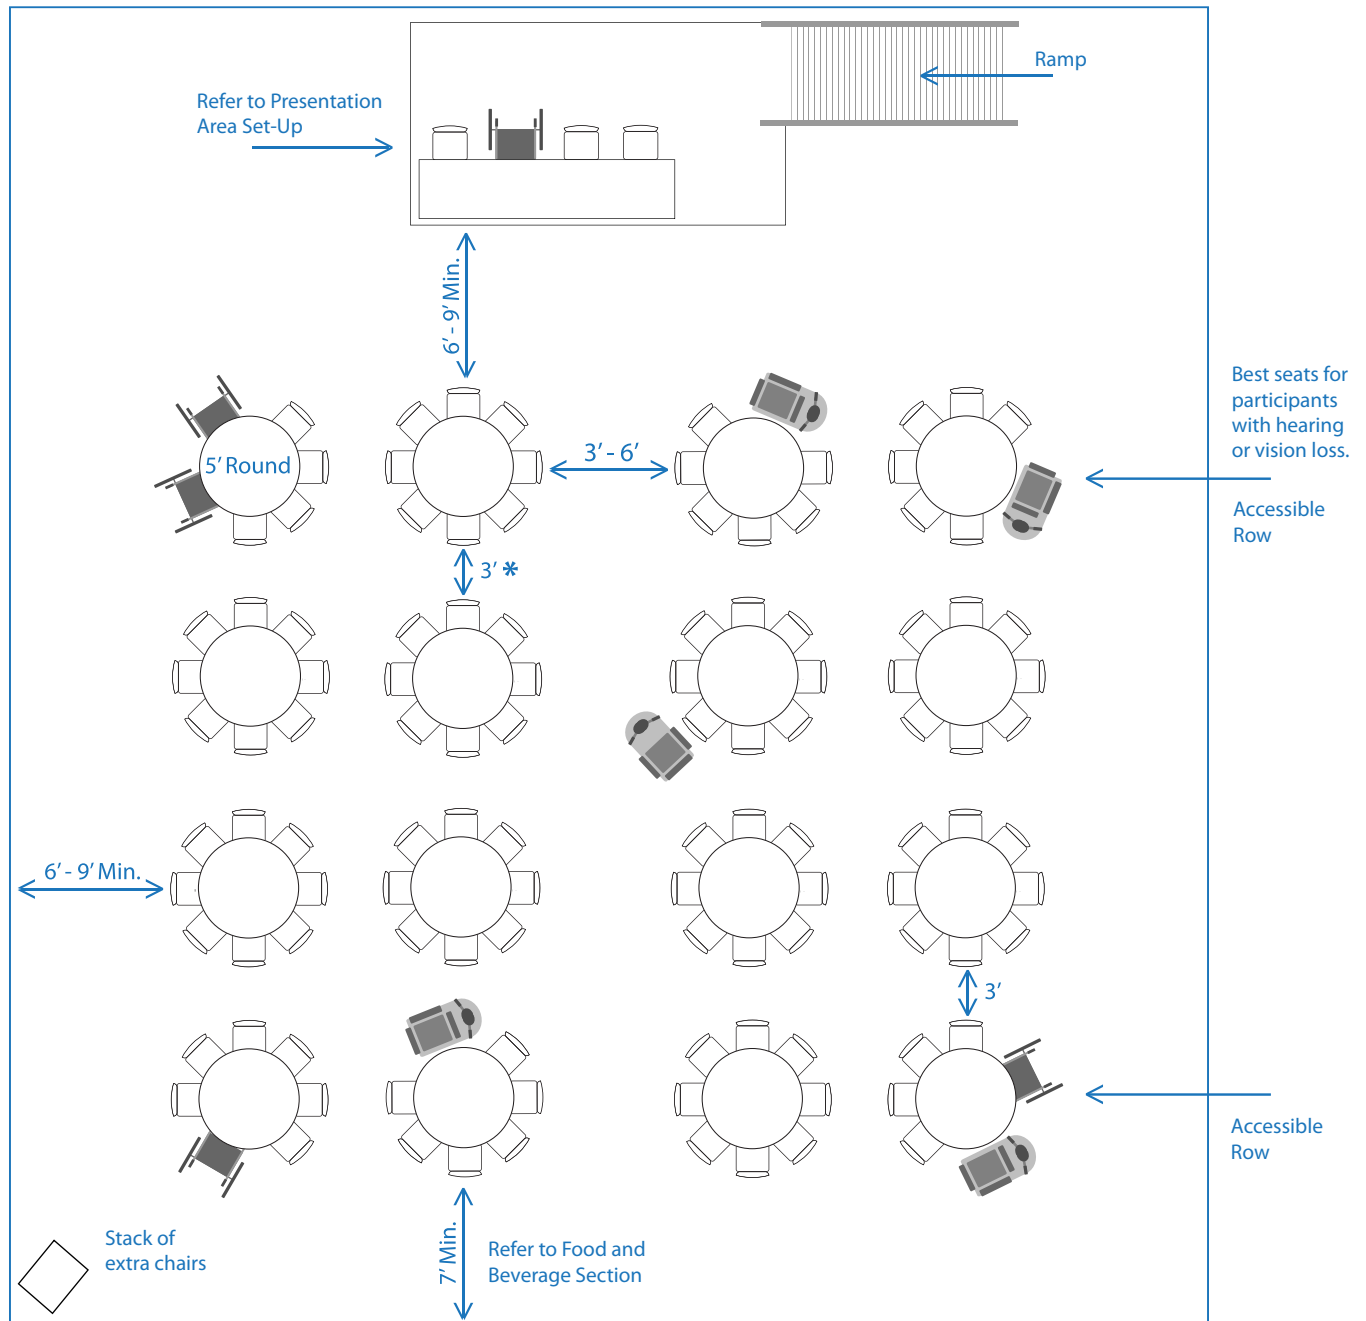